

# TIMS: Long Term Reproducibility of Nd Isotopic Data Acquired on TRITON *Plus*


Anne Trinquier, Thermo Fisher Scientific, Bremen, Germany

## Key Words

Neodymium, TRITON *Plus* TIMS, Static Mode, Virtual Amplifier,  $10^{11}\Omega$  Amplifier

## Introduction

Neodymium is a rare earth metal with seven naturally occurring isotopes:  $^{142}\text{Nd}$  (27.2%),  $^{143}\text{Nd}$  (12.2%),  $^{144}\text{Nd}$  (23.8%),  $^{145}\text{Nd}$  (8.3%),  $^{146}\text{Nd}$  (17.2%),  $^{148}\text{Nd}$  (5.7%) and  $^{150}\text{Nd}$  (5.6%). The ability to resolve Nd isotopic anomalies at the ppm level in materials with a wide range of Nd concentrations is essential for investigating fundamental relations in geochronology, geochemistry, cosmochemistry and environmental sciences. Neodymium isotope Thermal Ionization Mass Spectrometry (TIMS) has proven successful in running Nd both as  $\text{Nd}^+$  on multiple filament assemblies<sup>1,2</sup> (300–500 ng) and  $\text{NdO}^+$  on single filament assemblies<sup>3,4</sup> (1–10 ng). With the advent of second-generation TIMS instruments in the late 1990's, the reproducibility of Nd isotopic analyses improved by an order of magnitude, down to 2 ppm/amu (ref. 1), thus improving time resolution of geochronology by a factor of 3. Subsequent publications show a gross inter-laboratory consensus on a typical external reproducibility on the order of 2–5 ppm/amu on 500 ng  $\text{Nd}^+$  loads. The present study on a Thermo Scientific™ TRITON *Plus*™ TIMS assesses the precision and reproducibility over 1 year of Nd isotope analyses in metal form ( $\text{Nd}^+$ ) on double filament assemblies on one Nd standard (Merck #170335) for sample loads ranging from 500 ng to 100 ng, using  $10^{11}\Omega$  amplifiers, automated mode and analytical runs of about 1 hour.

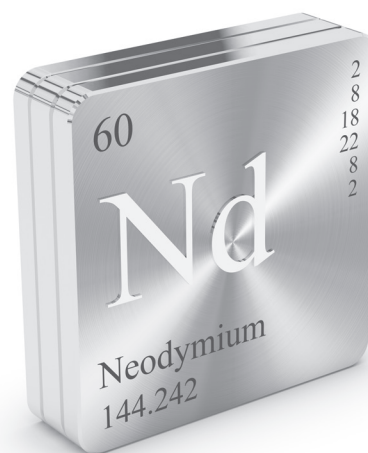

## The Virtual Amplifier

In static acquisition mode, the uncertainty on amplifier gain calibration propagates into the uncertainty of the isotopic ratio analysis. However, if, during analysis, all cups are sequentially connected to all amplifiers, all ion beams are in turn measured with the same set of amplifiers, and the stochastic calibration biases of the amplifiers can be averaged out. The virtual amplifier thus reduces the propagation of the uncertainty of the gain calibration procedure. The switching of amplifier-cup associations is performed as an inter-block action in a few ms. To ensure association of all Faraday cups with all amplifiers, the number of data blocks should be a multiple of the number of active amplifiers.<sup>5</sup>

## Analytical Protocol

### Neodymium Static Analysis with Virtual Amplifier

|   |   |
|---|---|
| Isotopic Standard                         | MERCK Neodymium ICP standard 170335<br>$^{143}\text{Nd}/^{144}\text{Nd} = 0.512399 \pm 3$ (2SD)*  |
| Filament Assembly                         | Zone refined rhenium double filaments   |
| Outgasing                                 | 40 minutes at 3.2 A; 10 minutes at 4.5 A  |
| Loading                                   | Nd in 6M HCl  |
| Additives                                 | 1 $\mu\text{L}$ 0.3M $\text{H}_3\text{PO}_4$<br>Dull red glow for 5 s   |
| Amount and Signal                         | 500 ng, 2–9 V $^{142}\text{Nd}$   |
| Acquisition Mode                          | Static, virtual amplifier: 3 cycles of rotation (480 ratios) or 2 cycles of rotation (320 ratios), sequence   |
| Baseline                                  | 105 s before each block   |
| Temperature ( $^{\circ}\text{C}$ )        | 1650 $^{\circ}\text{C}$ on the ionization filament  |
| Normalized to                             | $^{146}\text{Nd}/^{144}\text{Nd} = 0.7219$ , exponential correction   |
| Internal Precision (2RSE)                 | 6 ppm on $^{143}\text{Nd}/^{144}\text{Nd}$ (5 V $^{142}\text{Nd}$ , 480 ratios, ca. 1.5 h acquisition); 5 ppm on $^{143}\text{Nd}/^{144}\text{Nd}$ (10 V $^{142}\text{Nd}$ , 320 ratios, ca. 1 h acquisition) |
| Long-Term External Reproducibility (2RSD) | 2 to 6 ppm/amu on 100 and 500 ng loads (n=73, 1 year)   |

\* TRITON *Plus*, Thermo Fisher Scientific, Bremen, Application Laboratory (100–500 ng loads; n=73).

Table 1. Cup configuration.

| Line No. | Mass Set | L3                | L2                | L1                | RPQ/IC1 C         | H1                | H2                | H3                | H4                | Integration Time(s) | Number of Integrations | Idle Time(s) | Control Cup Peakcenter | Control Cup Focus |
|----------|----------|-------------------|-------------------|-------------------|-------------------|-------------------|-------------------|-------------------|-------------------|---------------------|------------------------|--------------|------------------------|-------------------|
| 1        | Main     | $^{142}\text{Nd}$ | $^{143}\text{Nd}$ | $^{144}\text{Nd}$ | $^{145}\text{Nd}$ | $^{146}\text{Nd}$ | $^{147}\text{Sm}$ | $^{148}\text{Nd}$ | $^{150}\text{Nd}$ | 8.389               | 1                      | 5.000        | $^{145}\text{Nd}$      | $^{142}\text{Nd}$ |

## External Reproducibility

Nd isotope ratios corrected for instrumental mass bias are plotted in Figure 1. Nd<sup>+</sup> analyses of 500 ng and 100 ng loads on double Re filament assemblies in static mode with rotation of the amplifier-cup association (“virtual amplifier”) yield indistinguishable isotopic ratios. The 1-yr 2RSD reproducibility on 100 ng and 500 ng loads is 2 to 6 ppm/amu (n=73, 3.6-10 V <sup>142</sup>Nd<sup>+</sup>). Notably, analyses with 10 V <sup>142</sup>Nd<sup>+</sup> ion beams can be limited to 1 hr and analyses with 100 ng to 1 h 30.

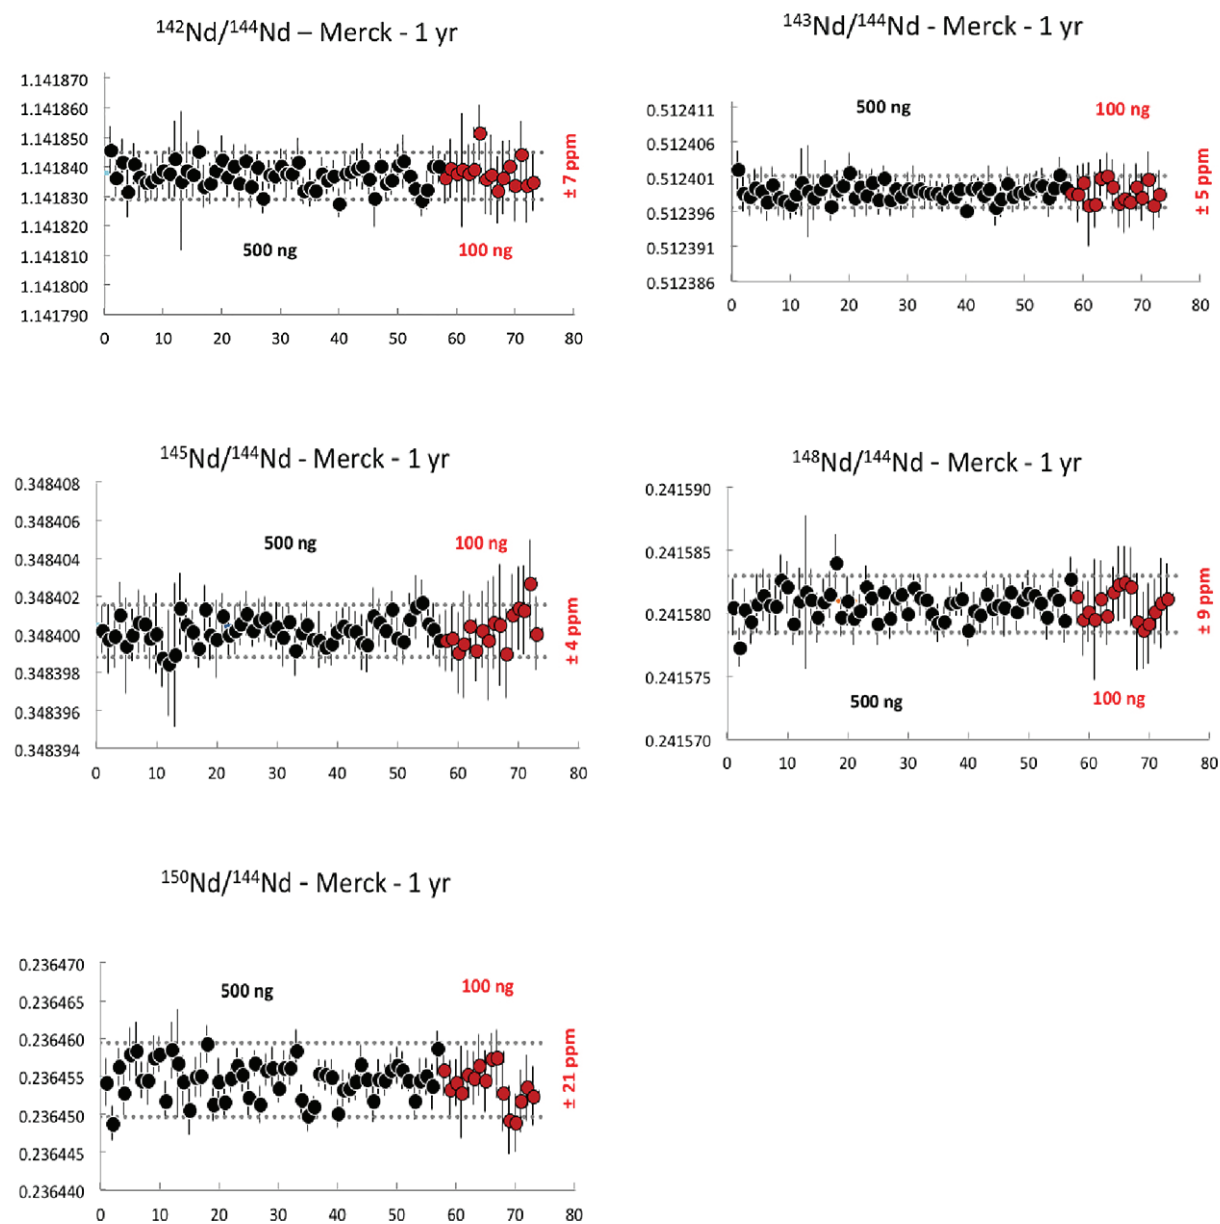


Figure 1. <sup>142</sup>Nd/<sup>144</sup>Nd 2SD 1 year long-term external reproducibility of Nd metal analyses using the virtual amplifier. One year 2RSD reproducibility on 500 ng loads: 2 to 5 ppm/amu (n=57, no outlier, 2-10 V <sup>142</sup>Nd<sup>+</sup>, 3 and 2 cycles of amplifier-cup rotation). 2 cycles of amplifier rotation at <sup>142</sup>Nd = 9 V (1 h analysis) compared to 3 cycles at <sup>142</sup>Nd = 5 V (1 h 30 min analysis). 2RSD reproducibility on 100 ng loads = 2 to 6 ppm/amu (n=16, no outlier, 3.6 V <sup>142</sup>Nd<sup>+</sup>, 3 cycles of amplifier-cup rotation). Error bars are 2se.

## Conclusion

Twice faster Nd isotopic analyses compared to literature can be achieved in static mode with virtual amplifier. One hour-long analyses yield a 2SD 1 year external reproducibility of 2 to 5 ppm/amu, similar to external reproducibility obtained in literature. This validates the stability of the current amplifier system and the Faraday cup multiple collection system and supports routine analysis to high precision.

## References

1. Caro et al. 2003 *Nature* 423, 428-432.
2. Boyet and Carlson 2005 *Science* 309, 576-581.
3. Delmonte et al. 2008 *Geophys. Res. Lett.* 35, L07703.
4. Harvey and Baxter 2009 *Chem. Geol.* 258, 251-257.
5. Tuttas and Schwieters, Thermo Fisher Scientific Application Note 30015.

## [thermoscientific.com/TritonPlus](http://thermoscientific.com/TritonPlus)

©2014 Thermo Fisher Scientific Inc. All rights reserved. ISO is a trademark of the International Standards Organization. MERCK is a trademark of Merck KGaA. All other trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries. Specifications, terms and pricing are subject to change. Not all products are available in all countries. Please consult your local sales representative for details.

|  |                                       |                                      |                                     |
|--|---------------------------------------|--------------------------------------|-------------------------------------|
| <b>Africa</b> +43 1 333 50 34 0                                | <b>Denmark</b> +45 70 23 62 60        | <b>Japan</b> +81 45 453 9100         | <b>Singapore</b> +65 6289 1190      |
| <b>Australia</b> +61 3 9757 4300                               | <b>Europe-Other</b> +43 1 333 50 34 0 | <b>Latin America</b> +1 561 688 8700 | <b>Spain</b> +34 914 845 965        |
| <b>Austria</b> +43 810 282 206                                 | <b>Finland</b> +358 9 3291 0200       | <b>Middle East</b> +43 1 333 50 34 0 | <b>Sweden</b> +46 8 556 468 00      |
| <b>Belgium</b> +32 53 73 42 41                                 | <b>France</b> +33 1 60 92 48 00       | <b>Netherlands</b> +31 76 579 55 55  | <b>Switzerland</b> +41 61 716 77 00 |
| <b>Canada</b> +1 800 530 8447                                  | <b>Germany</b> +49 6103 408 1014      | <b>New Zealand</b> +64 9 980 6700    | <b>UK</b> +44 1442 233555           |
| <b>China</b> 800 810 5118 (free call domestic)<br>400 650 5118 | <b>India</b> +91 22 6742 9494         | <b>Norway</b> +46 8 556 468 00       | <b>USA</b> +1 800 532 4752          |
|  | <b>Italy</b> +39 02 950 591           | <b>Russia/CIS</b> +43 1 333 50 34 0  |                                     |

AN30280\_E 05/14S

**Thermo**  
SCIENTIFIC

A Thermo Fisher Scientific Brand